

User's Guide



Shop online at

www.omega.com

e-mail: info@omega.com



OME-PCI-1002

**PCI Data Acquisition Board
Windows Software Manual**



OMEGAnet® Online Service
www.omega.com

Internet e-mail
info@omega.com

Servicing North America:

USA:
ISO 9001 Certified

One Omega Drive, P.O. Box 4047
Stamford CT 06907-0047
TEL: (203) 359-1660 FAX: (203) 359-7700
e-mail: info@omega.com

Canada:

976 Bergar
Laval (Quebec) H7L 5A1, Canada
TEL: (514) 856-6928 FAX: (514) 856-6886
e-mail: info@omega.ca

For immediate technical or application assistance:

USA and Canada: Sales Service: 1-800-826-6342 / 1-800-TC-OMEGA®
Customer Service: 1-800-622-2378 / 1-800-622-BEST®
Engineering Service: 1-800-872-9436 / 1-800-USA-WHEN®
TELEX: 996404 EASYLINK: 62968934 CABLE: OMEGA

Mexico:

En Español: (001) 203-359-7803 e-mail: espanol@omega.com
FAX: (001) 203-359-7807 info@omega.com.mx

Servicing Europe:

Benelux:

Postbus 8034, 1180 LA Amstelveen, The Netherlands
TEL: +31 (0)20 3472121 FAX: +31 (0)20 6434643
Toll Free in Benelux: 0800 0993344
e-mail: sales@omegaeng.nl

Czech Republic:

Frystatska 184, 733 01 Karviná, Czech Republic
TEL: +420 (0)59 6311899 FAX: +420 (0)59 6311114
Toll Free: 0800-1-66342 e-mail: info@omegashop.cz

France:

11, rue Jacques Cartier, 78280 Guyancourt, France
TEL: +33 (0)1 61 37 29 00 FAX: +33 (0)1 30 57 54 27
Toll Free in France: 0800 466 342
e-mail: sales@omega.fr

Germany/Austria:

Daimlerstrasse 26, D-75392 Deckenpfronn, Germany
TEL: +49 (0)7056 9398-0 FAX: +49 (0)7056 9398-29
Toll Free in Germany: 0800 639 7678
e-mail: info@omega.de

United Kingdom:

ISO 9002 Certified

One Omega Drive, River Bend Technology Centre
Northbank, Irlam, Manchester
M44 5BD United Kingdom
TEL: +44 (0)161 777 6611 FAX: +44 (0)161 777 6622
Toll Free in United Kingdom: 0800-488-488
e-mail: sales@omega.co.uk

It is the policy of OMEGA to comply with all worldwide safety and EMC/EMI regulations that apply. OMEGA is constantly pursuing certification of its products to the European New Approach Directives. OMEGA will add the CE mark to every appropriate device upon certification.

The information contained in this document is believed to be correct, but OMEGA Engineering, Inc. accepts no liability for any errors it contains, and reserves the right to alter specifications without notice.

WARNING: These products are not designed for use in, and should not be used for, patient-connected applications.

Table of Contents

1.	Introduction	4
1.1	Software Installation	5
1.2	References	7
2.	Declaration Files	8
2.1	P100X.H	9
2.2	P100Xu.C	11
2.3	P100X.BAS	12
2.4	P100Xu.BAS	14
2.5	P100X.PAS	15
2.6	P100Xu.PAS	18
3.	Demo Result	19
3.1	Visual C++	19
3.2	Visual Basic	20
3.3	Delphi	21
3.4	Borland C++ Builder	22
4.	Descriptions of Functions	23
4.1	The Configuration Code Table	25
4.2	The Test Functions	26
	P100X_FloatSub2	26
	P100X_ShortSub2	26
4.2.3	P100X_GetDllVersion	27
	P100X_GetDriverVersion	27
4.3	The DI/O Functions	28
	P100X_Di	28
	P100X_Do	28
4.4	The A/D Fixed-mode Functions	29
	P100X_SetChannelConfig	29
4.4.2	P100X_Polling	30
4.4.3	P100X_AdPolling	31
4.4.4	P100X_AdsPolling	32
4.4.5	P100X_AdsPacer	33
4.5	Driver Functions	34
	P100X_DriverInit	34
	P100X_DriverClose	34
4.5.3	P100X_GetConfigAddressSpace	35
	P100X_WhichBoardActive	35
4.5.5	P100X_ActiveBoard	36
	P100X_GetIrqNo	36
4.6	The Interrupt Functions	37
	P100X_InstallIrq	37
	P100X_GetIntCount	37
4.6.3	P100X_INT_AdStart	38
	P100X_INT_AdStop	38
4.6.5	P100X_GetBuffer	39
	P100X_GetFloatBuffer	39
4.6.7	Architecture of Interrupt mode	40
5.	Program Architecture	44
6.	Reporting Problems	45

1. Introduction

The **OME-PCI-1002 Toolkit** is a collection of DLLs and device-driver for Windows 95/98/NT/2000/XP applications. These DLLs are 32-bit and can be called by Visual C++, BC++, Visual BASIC, Delphi and LabVIEW.

The OME-PCI-1002 Toolkit consists of the following DLLs and device driver:


- P100X.DLL, P100X.LIB → for OME-PCI-1002 card
- P100X.VXD → OME-PCI-1002 Device driver for Windows 95/98
- P100X.SYS → OME-PCI-1002 Device driver for Windows NT/2000/XP

The DLLs perform a variety of tasks including:

- Read software version
- Initialization
- Digital Input/Output
- A/D conversion


1.1 Software Installation

Insert the CD ROM included with your OME-PCI-1002 board and the following installation screen should auto-start.

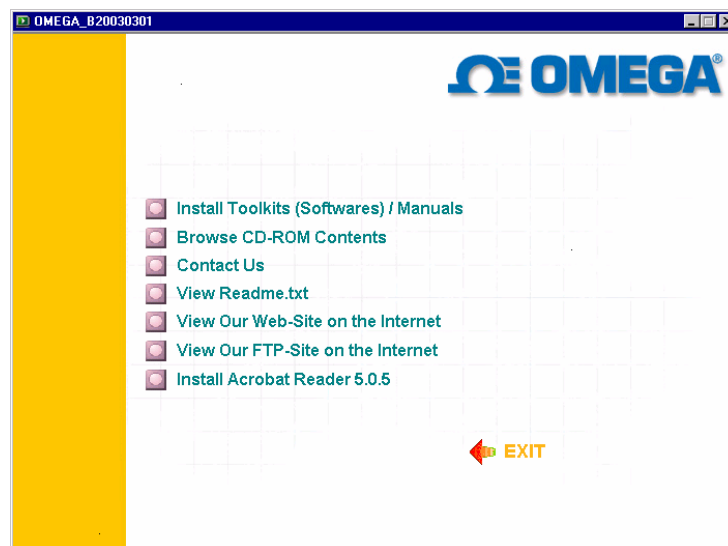

Follow the instructions on the screen to complete the software installation. The software is designed to support the entire OME family of data acquisition hardware, so during the installation, you will be asked to specify your particular hardware (OME-PCI-1002 board in this case). During the installation process, you will also be prompted to enter the operating system you will be using.

After installation the following folders will be created on your computer.

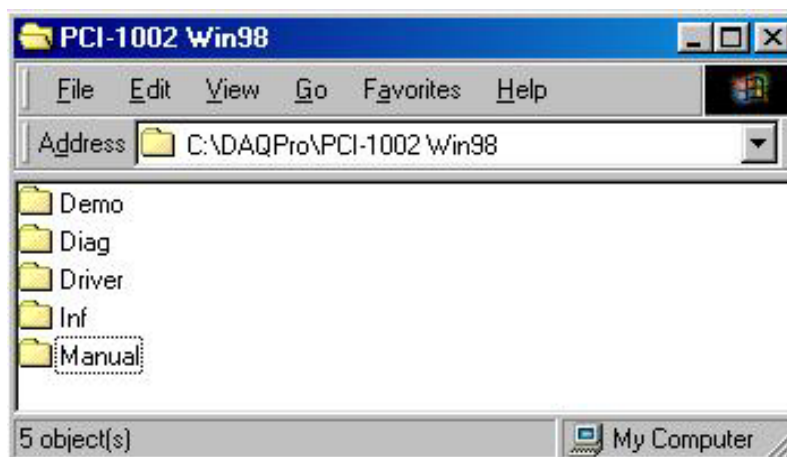

Demo Folder

Contains all demonstration programs including their source code. Examples are provided for Visual C++, Borland C++, Visual Basic and Delphi.

Please note: The VC++ demos are developed with VC++ 4.0. After setting up the environment, use the NMAKE.EXE to compiling and linking the demo code. For Example, C:\P1002\DEMO\VC\nmake /f demo.mak

Driver Folder

Contains software drivers, include files and definition files for the programming languages.

Manual Folder

Contains hardware user manuals, software user manuals and technical notes.

Diag Folder

Contains card diagnostic programs

Inf Folder

Contains tech notes and .INF file for the plug and play installation (only available for operating systems that support plug and play).

1.2 References

Please also refer to the following user manuals:

- **SoftInst.pdf:**
To install the software package under Windows 95/98/NT/2000/XP.
- **CallDll.pdf:**
To call the DLL functions with Visual C++, Visual Basic, Delphi and Borland C++.
- **ResCheck.pdf:**
To check the card resources, that is, I/O Port address, IRQ number and DMA under Windows.

2. Declaration Files

Please refer to user manual "[CalIDLL.pdf](#)".

--\Driver	← some device driver
--\VB	← for Visual Basic
--\P100X.BAS	← Declaration file for Visual Basic
--\P100Xu.BAS	← Functions for Visual Basic
--\VC	← for Visual C++
--\P100X.H	← Header file
--\P100X.LIB	← Import library for VC only
--\Delphi	← for Delphi
--\P100X.PAS	← Declaration file
--\P100Xu.PAS	← Functions for Delphi
--\BCB	← for Borland C++ Builder 3.0
--\P100X.H	← Header file
--\P100Xu.C	← Functions for BCB
--\P100X.LIB	← Import library file for BCB only

2.1 P100X.H

```
#ifdef __cplusplus
    #define EXPORTS extern "C" __declspec (dllimport)
#else
    #define EXPORTS
#endif

// return code
#define P100X_NoError 0
#define P100X_DriverHandleError 1
#define P100X_DriverCallError 2
#define P100X_AdControllerError 3
#define P100X_ConfigCodeError 4
#define P100X_DriverNoOpen 5
#define P100X_AdPollingTimeOut 6
#define P100X_FindBoardError 7
#define P100X_AdChannelError 8
#define P100X_DaChannelError 9
#define P100X_InvalidDelay 10
#define P100X_DelayTimeOut 11
#define P100X_InvalidData 12
#define P100X_TimeoutError 13
#define P100X_ExceedBoardNumber 14
#define P100X_NotFoundBoard 15
#define P100X_OpenError 16
#define P100X_FindTwoBoardError 17
#define P100X_GetIntCountError 18
#define P100X_InstallIrqError 19
#define P100X_AllocateMemoryError 20

EXPORTS float CALLBACK P100X_FloatSub(float fA, float fB);
EXPORTS short CALLBACK P100X_ShortSub(short nA, short nB);
EXPORTS WORD CALLBACK P100X_GetDllVersion(void);

EXPORTS WORD CALLBACK P100X_DriverInit(WORD *wTotalBoards);
EXPORTS void CALLBACK P100X_DriverClose(void);
EXPORTS WORD CALLBACK P100X_GetDriverVersion
    (WORD *wDriverVersion);
EXPORTS WORD CALLBACK P100X_GetIrqNo( WORD *IrqNo);

EXPORTS WORD CALLBACK P100X_GetConfigAddressSpace
    (WORD wBoardNo, WORD *wAddress0,
     WORD *wAddress1, WORD *wAddress2);

EXPORTS WORD CALLBACK P100X_ActiveBoard( WORD wBoardNo );
EXPORTS WORD CALLBACK P100X_WhichBoardActive(void);
```

```
EXPORTS void      CALLBACK P100X_SetupTimer
    (WORD wChannel, WORD wCoef);
EXPORTS WORD      CALLBACK P100X_Delay(WORD wDownCount);

EXPORTS void      CALLBACK P100X_Do(WORD wOutData);
EXPORTS WORD      CALLBACK P100X_Di(WORD *wDiData);

EXPORTS WORD      CALLBACK P100X_SetChannelConfig
    (WORD wAdChannel, WORD wConfig);
EXPORTS WORD      CALLBACK P100X_Polling(WORD *wAdVal);
EXPORTS WORD      CALLBACK P100X_AdPolling(float *fAdVal);
EXPORTS WORD      CALLBACK P100X_AdsPolling
    (float fAdVal[], WORD wNum);

EXPORTS WORD      CALLBACK P100X_AdsPacer
    (float fAdVal[], WORD wNum, WORD wSamplingDiv);

EXPORTS WORD      CALLBACK P100X_InstallIrq
    (HANDLE *hEvent, DWORD dwCount);
EXPORTS WORD      CALLBACK P100X_GetBuffer
    (DWORD dwNum, WORD wBuf[]);
EXPORTS WORD      CALLBACK P100X_GetFloatBuffer
    (DWORD dwNum, float fAdVal[]);

EXPORTS WORD      CALLBACK P100X_GetIntCount(DWORD *dwVal);
EXPORTS WORD      CALLBACK P100X_INT_AdStart
    (WORD Ch, WORD Gain, WORD wFreqDiv);

EXPORTS WORD      CALLBACK P100X_INT_AdStop();
```

2.2 P100Xu.C

```
#include <math.h>
```

```

/*-----*
/* Return voltage value or -100.0 if any error occurs *
/* or parameter is out of range. *
/* HiLo : 1 --> High Gain , 0 --> Low Gain *
/* Gain : 0-3 *
/*-----*
float P100X_AD2F(Word hex, int HiLo,int Gain )
{
    float ZeroBase, VoltageRange, FullRange ;

    ZeroBase = 2048.0 ;
    FullRange = 2048.0 ;
    VoltageRange = 10.0 ;
    Gain = Gain % 16 ;
    if ( (Gain < 0) || (Gain > 3) )
        return -100.0;

    if ( HiLo == 0 ) //Low-Gain
        return (((hex - ZeroBase) / FullRange) * VoltageRange) / pow( 2 , Gain));
    else
        return (((hex - ZeroBase) / FullRange) * VoltageRange) / pow( 10 ,
Gain));
}

```

2.3 P100X.BAS

Attribute VB_Name = "P100X"

' return code

Global Const P100X_NoError	= 0
Global Const P100X_DriverHandleError	= 1
Global Const P100X_DriverCallError	= 2
Global Const P100X_AdControllerError	= 3
Global Const P100X_ConfigCodeError	= 4
Global Const P100X_DriverNoOpen	= 5
Global Const P100X_AdPollingTimeOut	= 6
Global Const P100X_FindBoardError	= 7
Global Const P100X_AdChannelError	= 8
Global Const P100X_DaChannelError	= 9
Global Const P100X_InvalidDelay	= 10
Global Const P100X_DelayTimeOut	= 11
Global Const P100X_InvalidData	= 12
Global Const P100X_TimeoutError	= 13
Global Const P100X_ExceedBoardNumber	= 14
Global Const P100X_NotFoundBoard	= 15
Global Const P100X_OpenError	= 16
Global Const P100X_FindTwoBoardError	= 17
Global Const P100X_GetIntCountError	= 18
Global Const P100X_InstallIrqError	= 19
Global Const P100X_AllocateMemoryError	= 20

' Function of Test

```
Declare Function P100X_FloatSub Lib "P100X.DLL" _
    (ByVal fA As Single, ByVal fB As Single) As Single
Declare Function P100X_ShortSub Lib "P100X.DLL" _
    (ByVal nA As Integer, ByVal nB As Integer) As Integer
Declare Function P100X_GetDllVersion Lib "P100X.DLL" () As Integer
```

' Function of Driver

```
Declare Function P100X_DriverInit Lib "P100X.DLL" _
    (wTotalBoards As Integer) As Integer
Declare Sub P100X_DriverClose Lib "P100X.DLL" ()
Declare Function P100X_GetDriverVersion Lib "P100X.DLL" _
    (wDriverVersion As Integer) As Integer
Declare Function P100X_GetIrqNo Lib "P100X.DLL" (IrqNo As Integer) _
    As Integer
Declare Function P100X_GetConfigAddressSpace Lib "P100X.DLL" _
    (ByVal wBoardNo As Integer, wAddrTimer As Integer, _
    wAddrDio As Integer, wAddrAd As Integer) As Integer
Declare Function P100X_ActiveBoard Lib "P100X.DLL" _
    (ByVal wBoardNo As Integer) As Integer
Declare Function P100X_WhichBoardActive Lib "P100X.DLL" () As Integer
```

```

Declare Sub P100X_SetupTimer Lib "P100X.DLL" _
    (ByVal wChannel As Integer, ByVal wCoef As Integer)
Declare Function P100X_Delay Lib "P100X.DLL" _
    (ByVal wDownCount As Integer) As Integer

' Function of DI/DO
Declare Sub P100X_Do Lib "P100X.DLL" (ByVal wOutData As Integer)
Declare Function P100X_Di Lib "P100X.DLL" (wDiData As Integer) As Integer

' Function of AD
Declare Function P100X_SetChannelConfig Lib "P100X.DLL" _
    (ByVal wAdChannel As Integer, ByVal wConfig As Integer) As Integer
Declare Function P100X_Polling Lib "P100X.DLL" _
    (wAdVal As Integer) As Integer
Declare Function P100X_AdPolling Lib "P100X.DLL" _
    (fAdVal As Single) As Integer
Declare Function P100X_AdsPolling Lib "P100X.DLL" _
    (fAdVal As Single, ByVal wNum As Integer) As Integer
Declare Function P100X_AdsPacer Lib "P100X.DLL" (fAdVal As Single, _
    ByVal wNum As Integer, ByVal wSamplingDiv As Integer) As Integer

' Function of Interrupt
Declare Function P100X_InstallIrq Lib "P100X.DLL" _
    (hEvent As Long, ByVal dwCount As Long) As Integer
Declare Function P100X_GetBuffer Lib "P100X.DLL" _
    (ByVal dwNum As Long, wBuf As Integer) As Integer
Declare Function P100X_GetFloatBuffer Lib "P100X.DLL" _
    (ByVal dwNum As Long, fAdVal As Single) As Integer
Declare Function P100X_INT_AdStart Lib "P100X.DLL" _
    (ByVal Ch As Integer, ByVal Gain As Integer, _
    ByVal wFreqDiv As Integer) As Integer
Declare Function P100X_INT_AdStop Lib "P100X.DLL" () As Integer
Declare Function P100X_GetIntCount Lib "P100X.DLL" (dwVal As Long) _
    As Integer

```

2.4 P100Xu.BAS

```

'*-----*
'* Return voltage value or -100.0 if any error occurs  *
'* or parameter is out of range.                      *
'* HiLo : 1 --> High Gain , 0 --> Low Gain            *
'* Gain : 0-3                                          *
'*-----*
Function P100X_AD2F(ByVal hex, HiLo, Gain As Integer) As Single
    Dim ZeroBase, FullRange, VoltageRange As Single

    ZeroBase = 2048#
    FullRange = 2048#
    VoltageRange = 10#
    Gain = Gain Mod 16

    If Gain < 0 Or Gain > 3 Then
        P100X_AD2F = -100#
        Exit Function
    End If

    If HiLo = 0 Then 'Low-Gain
        P100X_AD2F = (((hex - ZeroBase) / FullRange) * VoltageRange) / (2 ^
Gain))
    Else
        P100X_AD2F = (((hex - ZeroBase) / FullRange) * VoltageRange) / (10 ^
Gain))
    End If
End Function

```

2.5 P100X.PAS

```
unit P100X;
```

```
interface
```

```
type PSingle=^Single;
```

```
type PWord=^Word;
```

```
const
```

```
// return code
```

```
P100X_NoError           = 0;
P100X_DriverHandleError = 1;
P100X_DriverCallError   = 2;
P100X_AdControllerError = 3;
P100X_ConfigCodeError   = 4;
P100X_DriverNoOpen      = 5;
P100X_AdPollingTimeOut  = 6;
P100X_FindBoardError    = 7;
P100X_AdChannelError    = 8;
P100X_DaChannelError    = 9;
P100X_InvalidDelay      = 10;
P100X_DelayTimeOut      = 11;
P100X_InvalidData       = 12;
P100X_TimeoutError      = 13;
P100X_ExceedBoardNumber = 14;
P100X_NotFoundBoard     = 15;
P100X_OpenError         = 16;
P100X_FindTwoBoardError = 17;
P100X_GetIntCountError  = 18;
P100X_InstallIrqError   = 19;
P100X_AllocateMemoryError = 20;
```

```
// Function of Test
```

```
function P100X_FloatSub(fA:Single; fB:Single):Single ; stdCall;
```

```
function P100X_ShortSub(nA:SmallInt; nB:SmallInt):SmallInt ; stdCall;
```

```
function P100X_GetDllVersion:WORD ; stdCall;
```

```
// Function of Driver
function P100X_DriverInit(Var wTotalBoards:Word):WORD ; stdCall;
procedure P100X_DriverClose; stdCall;
function P100X_GetDriverVersion(var wDriverVersion:Word):WORD ; stdCall;
function P100X_GetIrqNo(Var IrqNo:WORD):WORD; StdCall;
function P100X_GetConfigAddressSpace(wBoardNo:Word;
    var wAddrTimer:Word; var wAddrDio:Word;
    var wAddrAd:Word) :WORD ; stdCall;
function P100X_ActiveBoard(wBoardNo:Word):WORD ; stdCall;
function P100X_WhichBoardActive:WORD ; stdCall;
procedure P100X_SetupTimer(wChannel:Word; wCoef:Word); stdCall;
function P100X_Delay(wDownCount:Word):Word; StdCall;

// Function of DI/DO
procedure P100X_Do(wOutData:Word); stdCall;
function P100X_Di(var wDiData:Word):WORD ; stdCall;

// Function of AD
function P100X_SetChannelConfig
    (wAdChannel:Word; wConfig:Word):WORD ; stdCall;
function P100X_Polling(var wAdVal:Word):WORD ; stdCall;
function P100X_AdPolling(var fAdVal:Single):WORD ; stdCall;
function P100X_AdsPolling(fAdVal:PSingle; wNum:Word):WORD ; stdCall;
function P100X_AdsPacer(fAdVal:PSingle; wNum:Word;
    wSamplingDiv:Word ):WORD ; stdCall;

// Function of Interrupt
function P100X_InstallIrq
    (Var hEvent:LongInt; dwCount: LongInt):WORD ; stdCall;
function P100X_GetBuffer(dwNum:LongInt;wBuf:PWord):WORD ; stdCall;
function P100X_GetFloatBuffer
    (dwNum:LongInt; fAdVal:PSingle):Word; StdCall;
function P100X_INT_AdStart
    (Ch:WORD; Gain:WORD; wFreqDiv:Word):WORD ; stdCall;
function P100X_INT_AdStop:WORD ; stdCall;
function P100X_GetIntCount(var dwVal:LongInt):WORD ; stdCall;
```

implementation

```
function 100X_FloatSub; external 'P100X.DLL' name 'P100X_FloatSub';
function 100X_ShortSub; external 'P100X.DLL' name 'P100X_ShortSub';
function 100X_GetDIIVersion;
    external 'P100X.DLL' name 'P100X_GetDIIVersion';
function 100X_GetDriverVersion;
    external 'P100X.DLL' name 'P100X_GetDriverVersion';
```

```

function      100X_DriverInit; external 'P100X.DLL' name 'P100X_DriverInit';
procedure    100X_DriverClose;
              external 'P100X.DLL'      name 'P100X_DriverClose';
function      100X_GetIrqNo; external 'P100X.DLL' name 'P100X_GetIrqNo';
function      100X_GetConfigAddressSpace;
              external 'P100X.DLL' name 'P100X_GetConfigAddressSpace';
function      100X_ActiveBoard;
              external 'P100X.DLL'      name 'P100X_ActiveBoard';
function      100X_WhichBoardActive;
              external 'P100X.DLL'      name 'P100X_WhichBoardActive';
procedure    100X_SetupTimer;
              external 'P100X.DLL'      name 'P100X_SetupTimer';
function      100X_Delay;    external 'P100X.DLL' name 'P100X_Delay';


procedure    P100X_Do;    external 'P100X.DLL' name 'P100X_Do';
function      P100X_Di;    external 'P100X.DLL' name 'P100X_Di';


function      P100X_SetChannelConfig;
              external 'P100X.DLL'      name 'P100X_SetChannelConfig';
function      P100X_Polling; external 'P100X.DLL' name 'P100X_Polling';
function      P100X_AdPolling;
              external 'P100X.DLL'      name 'P100X_AdPolling';
function      P100X_AdsPolling;
              external 'P100X.DLL'      name 'P100X_AdsPolling';


function      P100X_AdsPacer;
              external 'P100X.DLL'      name 'P100X_AdsPacer';


function      P100X_InstallIrq;
              external 'P100X.DLL'      name 'P100X_InstallIrq';
function      P100X_INT_AdStart;
              external 'P100X.DLL'      name 'P100X_INT_AdStart';
function      P100X_INT_AdStop;
              external 'P100X.DLL'      name 'P100X_INT_AdStop';
function      P100X_GetIntCount;
              external 'P100X.DLL'      name 'P100X_GetIntCount';
function      P100X_GetBuffer;
              external 'P100X.DLL'      name 'P100X_GetBuffer';
function      P100X_GetFloatBuffer;
              external 'P100X.DLL'      name 'P100X_GetFloatBuffer';

end.

```

2.6 P100Xu.PAS

unit P100Xu;

interface

Function P100X_AD2F(hex, HiLo, Gain :Word): Single ; StdCall;

implementation

uses math;

```

/*-----*
/* Return voltage value or -100.0 if any error occurs *
/* or parameter is out of range.
/* HiLo : 1 --> High Gain , 0 --> Low Gain
/* Gain : 0-3
/*-----*

```

Function P100X_AD2F(hex, HiLo, Gain :Word): Single ;

Var

ZeroBase, VoltageRange, FullRange : Single ;

Begin

ZeroBase := 2048;

FullRange := 2048;

VoltageRange := 10;

Gain := Gain mod 16;

If (Gain < 0) Or (Gain > 3) Then

begin

P100X_AD2F := -100;

exit;

end ;

If HiLo = 0 Then //Low-Gain

Result := (((hex - ZeroBase) / FullRange) * VoltageRange) / Power(2, Gain))

Else


Result := (((hex - ZeroBase) / FullRange) * VoltageRange) / Power(10, Gain));

End;


end.

3. Demo Result

3.1 Visual C++

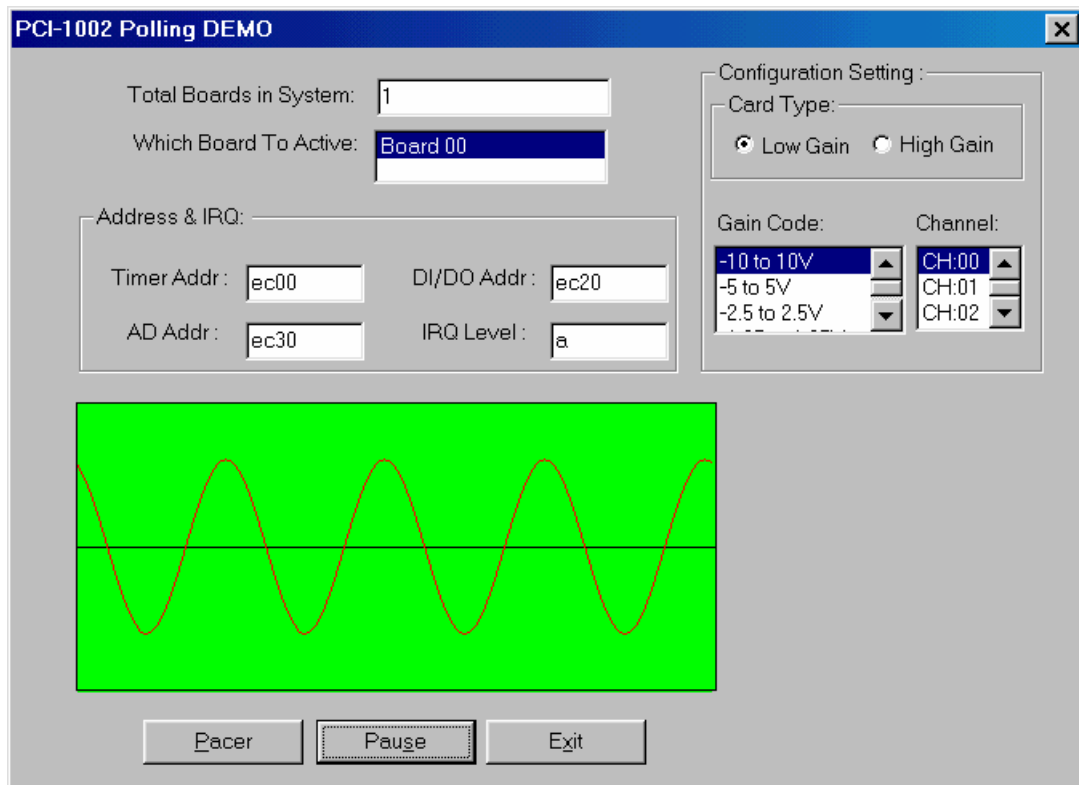


Analog Input with polling demo program

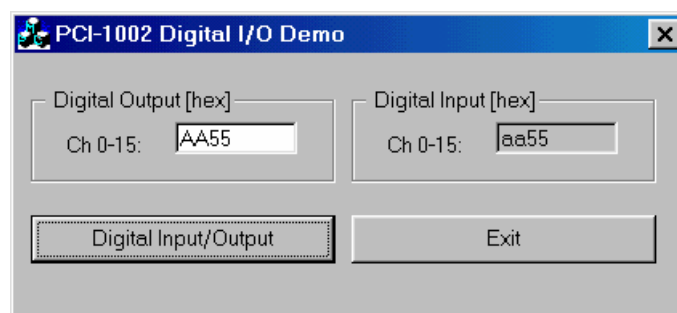


Digital I/O with MFC demo program

3.2 Visual Basic

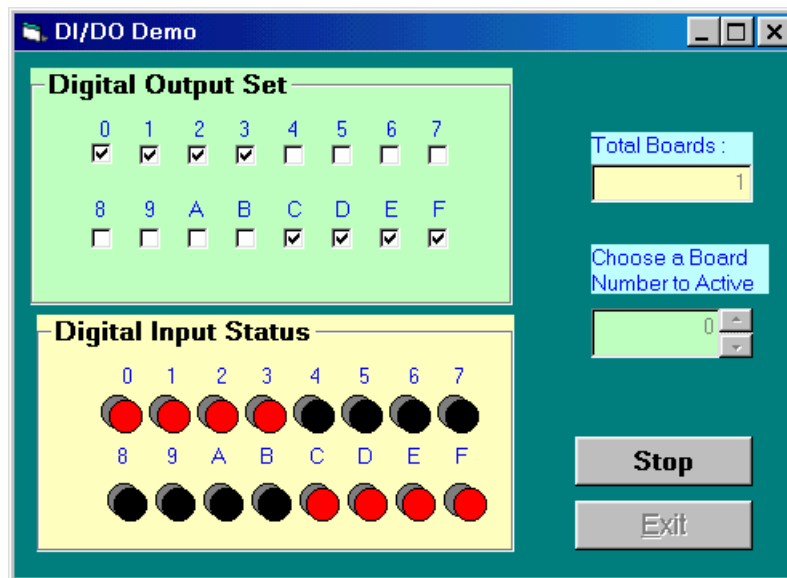


Digital I/O demo program

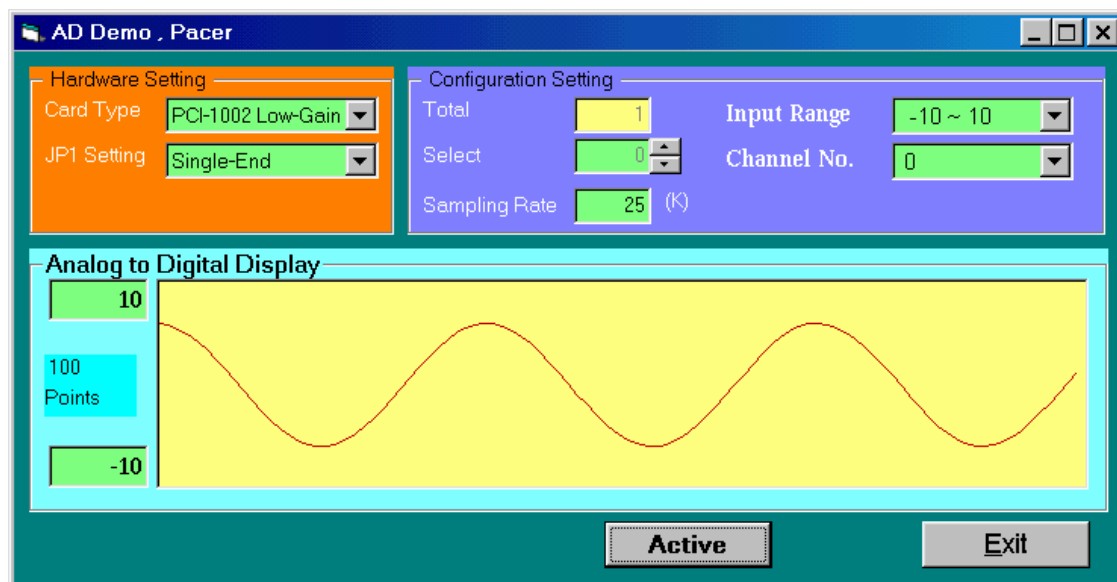


Analog Input with pacer-trigger demo program

3.3 Delphi

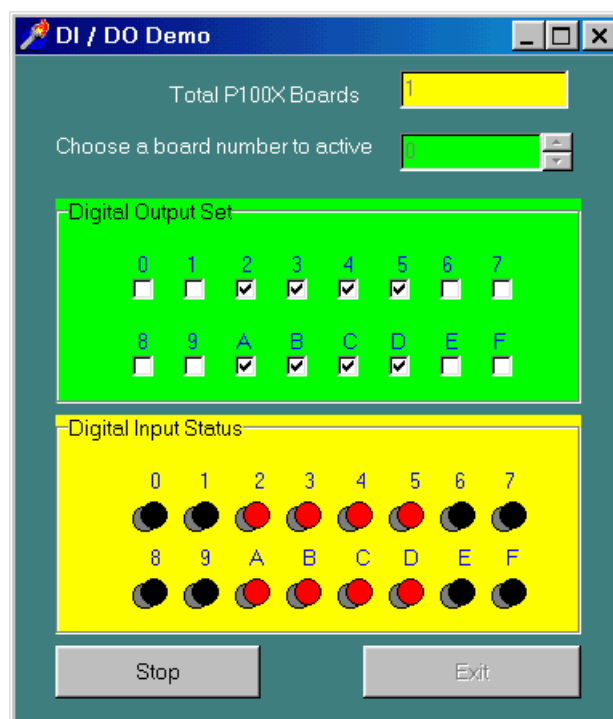


Digital I/O demo program

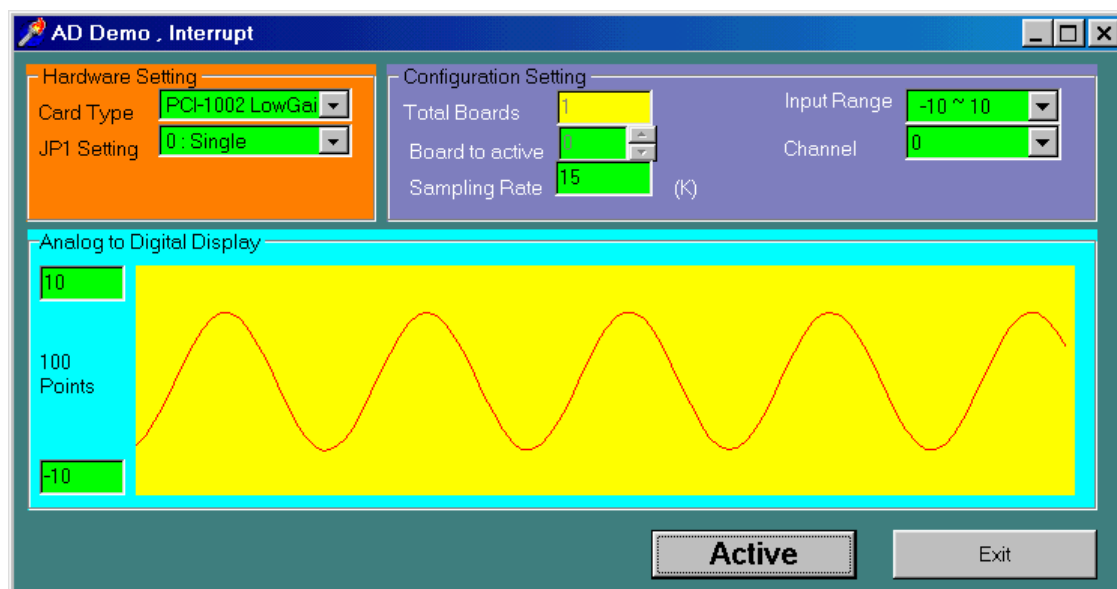


Analog Input with Interrupt demo program

3.4 Borland C++ Builder

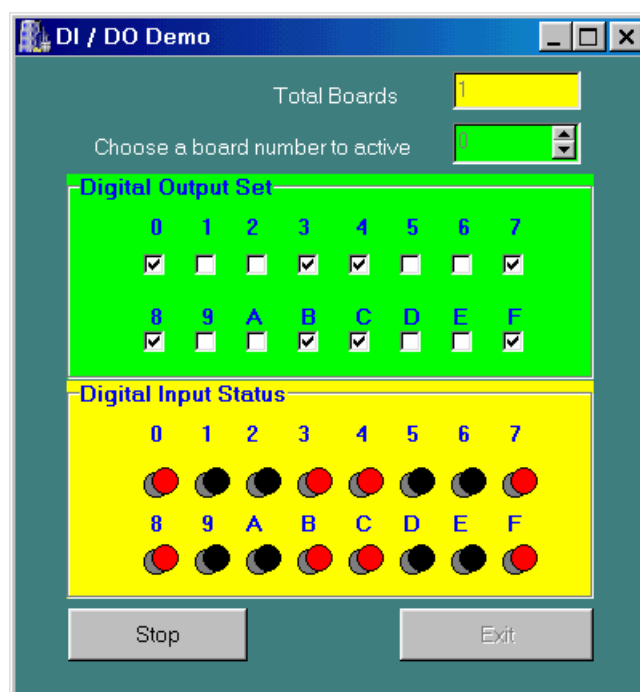

Digital I/O demo program

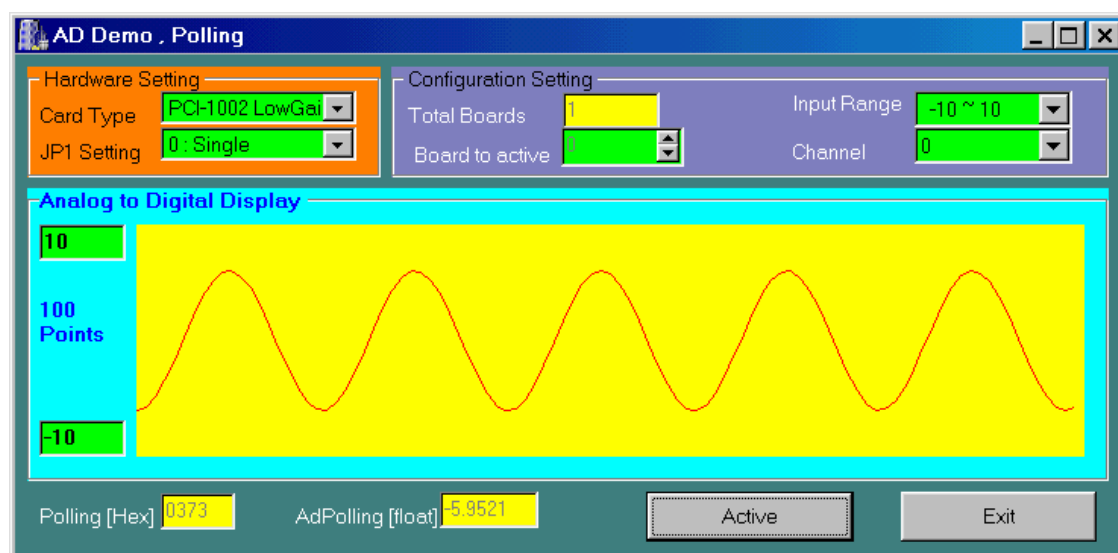

Analog input with polling demo program

4. Descriptions of Functions

The DLL functions are divided into the following groups:

- Test Functions
- D/I/O Functions
- A/D Fixed-mode Functions
- Driver Functions
- Interrupt Functions

Test Functions:

1. P100X_FloatSub2
2. P100X_ShortSub2
3. P100X_GetDIIVersion
4. P100X_GetDriverVersion

D/I/O Functions

1. P100X_DI
2. P100X_DO

A/D Fixed-mode Functions:

1. P100X_SetChannelConfig
2. P100X_Polling
3. P100X_AdPolling
4. P100X_AdsPolling
5. P100X_AdsPacer

Driver Functions:

1. P100X_DriverInit
2. P100X_DriverClose
3. P100X_GetConfigAddressSpace
4. P100X_WhichBoardActive
5. P100X_ActiveBoard
6. P100X_GetIrqNo

Interrupt Functions:

1. P100X_InstallIrq
2. P100X_INT_AdStart
3. P100X_INT_AdStop
4. P100X_GetIntCount
5. P100X_GetBuffer
6. P100X_GetFloatBuffer

The following keywords are used to describe the attributes of function parameters.

Keyword	Parameter set by user before calling function?	Data/value available from this parameter after calling function?
[Input]	Yes	No
[Output]	No	Yes
[Input, Output]	Yes	Yes

4.1 The Configuration Code Table

OME-PCI-1002L Configuration Code Table

Gain	Bipolar	Max. Switching Frequency	Configuration Code
1	+/- 10V	110 K/S	0x00
2	+/- 5.0V	110 K/S	0x01
4	+/- 2.5V	110 K/S	0x02
8	+/- 1.25V	110 K/S	0x03

OME-PCI-1002H Configuration Code Table

Gain	Bipolar	Max. Switching Frequency	Configuration Code
1	+/- 10V	44 K/S	0x10
10	+/- 1.0V	36 K/S	0x11
100	+/- 0.1V	7 K/S	0x12
1000	+/- 0.01V	0.8 K/S	0x13

4.2 The Test Functions

4.2.1 P100X_FloatSub2

- **Description:**
Calculates $C = fA - fB$ in **float** format, **float=4 bytes floating point number**. This function is provided to test DLL linkage.
- **Syntax:**
`float P100X_FloatSub2(float fA, float fB);`
- **Parameter:**
fA : [Input] 4 bytes floating point value
fB : [Input] 4 bytes floating point value
- **Return:**
Returns the result value ($= fA - fB$).

4.2.2 P100X_ShortSub2

- **Description :**
Calculates $C = nA - nB$ in SHORT formats, **SHORT=16 bits signed number**. This function is provided to test DLL linkage.
- **Syntax :**
`short P100X_ShortSub2(Short nA, Short nB);`
- **Parameter:**
nA : [Input] 16-bit value
nB : [Input] 16-bit value
- **Return:**
Returns the result value ($= nA - nB$).

4.2.3 P100X_GetDllVersion

- **Description :**
Reads the DLL version of the **P100X.DLL**.
- **Syntax :**
WORD P100X_GetDllVersion(void);
- **Parameter:**
None
- **Return:**
Returns the version of the DLL for Device-Driver.
return=0x200 → Version 2.0

4.2.4 P100X_GetDriverVersion

- **Description :**
This subroutine will read the software version of the P100X.VxD for Windows 95 or P100X.SYS of Windows NT/2000/XP.
- **Syntax :**
WORD P100X_GetDriverVersion(WORD *wDriverVersion);
- **Parameter:**
wDriverVersion : [Output] address of **wDriverVersion**,
which contains the version of Device-Driver.
wDriverVersion=0x200 → Version 2.0
- **Return:**
P100X_NoError : OK
P100X_DriverHandleError : P100X.VxD open error for Windows 95
P100X.SYS open error for Windows
NT/2000/XP
P100X_DriverCallError : call P100X.VxD return error
call P100X.SYS return error

4.3 The DI/O Functions

4.3.1 P100X_Di

- **Description :**

This subroutine will read the 16 bit data from the DI(digital input) port. This function addresses the current active OME-PCI-1002 board. Use the P100X_ActiveBoard(...) to select the active board.

- **Syntax :**

WORD P100X_Di(WORD *wDi);

- **Parameter:**

wDi : [Output] address of **wDi**,
which contains the 16 bits of digital input data .

- **Return:**

P100X_NoError : OK
P100X_FindBoardError : cannot find the OME-PCI-100X board
P100X_ExceedBoardNumber: invalid board number

4.3.2 P100X_Do

- **Description :**

This subroutine will write the 16 bit data to the DO(digital output) port. This function addresses the current active OME-PCI-1002 board. Use the P100X_ActiveBoard(...) to select the active board.

- **Syntax :**

WORD P100X_Do(WORD wDo);

- **Parameter:**

wDo : [Input] the 16-bit data sent to the digital-output port

- **Return:**

P100X_NoError : OK
P100X_ExceedBoardNumber : invalid board number
P100X_FindBoardError : cannot find OME-PCI-1002 board

4.4 The A/D Fixed-mode Functions

4.4.1 P100X_SetChannelConfig

- **Description :**

This function will set the A/D channel configuration code. This function will also set the active A/D channel for **P100X_AdPolling**, **P100X_AdsPolling** and **P100X_AdsPacer** functions. The function addresses the current active OME-PCI-1002 board. Use the P100X_ActiveBoard(...) to select the active board.

- **Syntax :**

WORD P100X_SetChannelConfig(WORD wChannel, WORD wConfig);

- **Parameter:**

wChannel : [Input] A/D channel number
wConfig : [Input] Configuration code. Refer to Sec. 3.1 for details.

- **Return:**

P100X_NoError : OK
P100X_ExceedBoardNumber: invalid board number
P100X_FindBoardError : can not find the OME-PCI-1002 board
P100X_AdControllerError : MagicScan controller
hardware handshake error

4.4.2 P100X_Polling

- **Description :**

Performs a single A/D conversion on the active channel by software polling. The **P100X_SetChannelConfig** subroutine can be used to change the channel or configuration code. Use the **P100X_ActiveBoard(...)** to select the active board.

- **Syntax :**

WORD P100X_Polling(word *wAdVal);

- **Parameter:**

wAdVal : [Output] address of **wAdVal**, which contains the A/D data
Data is returned as an integer value in the range 0-4095.

- **Return:**

P100X_NoError : OK
P100X_ExceedBoardNumber: invalid board number
P100X_FindBoardError : can not find the OME-PCI-1002 board
P100X_AdPollingTimeOut : hardware timeout error

4.4.3 P100X_AdPolling

- **Description :**

This subroutine will perform a single A/D conversion by polling. The **P100X_SetChannelConfig** function can be used to change the channel or configuration code. This function addresses the current active OME-PCI-1002 board. Use the **P100X_ActiveBoard(...)** function to select the active board.

- **Syntax :**

WORD P100X_AdPolling(float *fAdVal);

- **Parameter:**

fAdVal : [Output] address of **fAdVal**, which contains the AD data. The data is automatically converted to voltage based on the settings of **P100X_SetChannelConfig()**.

- **Return:**

P100X_NoError : OK
 P100X_ExceedBoardNumber: invalid board number
 P100X_FindBoardError : cannot find the OME-PCI-1002 board
 P100X_AdPollingTimeOut : hardware timeout error

4.4.4 P100X_AdsPolling

- **Description :**

Performs multiple A/D conversions on a single channel by polling. The **P100X_SetChannelConfig** subroutine can be used to change the channel or configuration code. This function addresses the current active OME-PCI-1002 board. Use P100X_ActiveBoard(...) to select the active board.

Since software polling can be interrupted by the operating system, the P100X_AdsPacer function is recommended when precisely reconstructing the waveform is desired.

- **Syntax :**

WORD P100X_AdsPolling(float fAdVal[], WORD wNum);

- **Parameter:**

fAdVal : [**Output**] starting address of the A/D data buffer(Array of float)
The data is converted to voltage based on the setting of the **P100X_SetChannelConfig()** function.

The user must allocate sufficient space for the buffer. The user can access the data after calling the function.

wNum : [**Input**] number of A/D conversions to be performed.

- **Return:**

P100X_NoError : OK
P100X_ExceedBoardNumber : Invalid board number
P100X_FindBoardError : Can not find the OME-PCI-1002 board
P100X_AdPollingTimeOut : Hardware timeout error

4.4.5 P100X_AdsPacer

- **Description :**

This function performs multiple A/D conversions on a single channel by pacer trigger. The **P100X_SetChannelConfig** function can be used to change the channel or configuration code. The function addresses the current active OME-PCI-1002 board. Use **P100X_ActiveBoard(...)** to select the active board.

- **Syntax :**

WORD P100X_AdsPacer(float fAdVal[], WORD wNum, WORD wSample);

- **Parameter:**

fAdVal : [Output] Address of the A/D data buffer (Array of WORD), data will be converted to voltage based on the settings of **P100X_SetChannelConfig()**.
The user must allocate sufficient space for the buffer. The user can access the data after calling the function.

wNum : [Input] number of AD conversions to be performed.

wSample : [Input] **AD sampling rate = 2M/wSample.**

- **Return:**

P100X_NoError : OK

P100X_ExceedBoardNumber: invalid board number

P100X_FindBoardError : cannot find the OME-PCI-1002 board

P100X_AdPollingTimeOut : hardware timeout error

4.5 Driver Functions

4.5.1 P100X_DriverInit

- **Description :**
This function will detect all OME-PCI-1002 boards installed in the system. This function must be called once before the other functions are called.
 - **Syntax :**
WORD P100X_DriverInit(WORD *wTotalBoard);
 - **Parameter:**
wTotalBoard : [Output] Address of **wTotalBoard**, which will contain the number of OME-PCI-1002 boards in the system.
wTotalBoard=0 → Not found.
wTotalBoard=1 → one OME-PCI-1002 card in the system
wTotalBoard=n → n OME-PCI-1002 cards in the system
 - **Return:**

P100X_NoError	: OK
P100X_NoFoundBoard	: can not detect any OME-PCI-1002
P100X_FindBoardError	: handshake check error
P100X_DriverHandleError	: the P100X.VxD .open error for Windows 95 the P100X.SYS .open error for Windows NT
P100X_DriverCallError	: call P100X.VxD return error call P100X.SYS return error
-

4.5.2 P100X_DriverClose

- **Description :**
Releases all system resources. This function should be called before terminating the program.
 - **Syntax :**
void P100X_DriverClose(void);
 - **Parameter:**
None
 - **Return:**
None
-

4.5.3 P100X_GetConfigAddressSpace

- **Description :**
Get the I/O address of OME-PCI-1002 board n. This function is for debugging purposes. It is not normally necessary to call this function.
- **Syntax :**
WORD P100X_GetConfigAddressSpace(WORD wBoardNo,
WORD *wAddrTimer, WORD *wAddrDio, WORD *wAddrAd);
- **Parameter:**
wBoardNo : [Input] OME-PCI-1002 board number
wAddrTimer, wAddrDio, wAddrAd : [Output] Address of wAddrTimer, wAddrDio, wAddrAD stores the address of the Timer, DI/DO and A/D.
Please refer to Hardware manual for additional details.
- **Return:**
P100X_NoError : OK
P100X_FindBoardError : handshake check error
P100X_ExceedBoardError : wBoardNo is invalidd

4.5.4 P100X_WhichBoardActive

- **Description:**
Returns the board number of the active board.
- **Syntax:**
WORD P100X_WhichBoardActive(void);
- **Parameter:**
None
- **Return:**
Returns the board number of the active board.

4.5.5 P100X_ActiveBoard

- **Description:**
This function makes a board active. This function must be called once before the D/I/O, A/D or D/A functions are called.
- **Syntax:**
WORD P100X_ActiveBoard(WORD wBoardNo);
- **Parameter:**
wBoardNo [Input] The board number of the board to make active
- **Return:**
P100X_NoError : OK
P100X_ExceedBoardError : wBoardNo is invalid

4.5.6 P100X_GetIrqNo

- **Description:**
This function will get the IRQ number of the active OME-PCI-1002 board installed in the system. This function is not normally used by user applications.
- **Syntax:**
WORD P100X_GetIrqNo(WORD *IrqNo);
- **Parameter:**
IrqNo : [Output] Address of IrqNo, which contains the IRQ No allocated by the system.
- **Return:**
P100X_NoError : OK

4.6 The Interrupt Functions

4.6.1 P100X_InstallIrq

- **Description :**

This subroutine will install the interrupt handler for a specific IRQ n. and set the maximum number of interrupts. Refer to section 3.6.7. for more details on using interrupts

- **Syntax :**

WORD P100X_InstallIrq(HANDLE *hEvent, DWORD dwCount);

- **Parameter:**

hEvent : [Input] The user must use the CreateEvent() to create the Event object and obtain its handle and pass the handle to this function.
dwCount : [Input] Maximum number of counts for interrupt transfer.

- **Return:**

P100X_NoError : successful
P100X_InstallIrqError : failed installing the IRQ handler.

4.6.2 P100X_GetIntCount

- **Description :**

This subroutine will read the interrupt transfer count.

- **Syntax :**

WORD P100X_GetIntCount(DWORD *dwVal)

- **Parameter:**

dwVal : [Output] the address of dwVal, which contains the value of interrupt transferred count.

- **Return:**

P100X_NoError : successful
P100X_GetIntCountError : fail get interrupt count.

4.6.3 P100X_INT_AdStart

- **Description :**

This subroutine will start the interrupt transfer for a specific A/D channel, set the gain code and sample rate.

- **Syntax :**

WORD P100X_INT_AdStart(WORD Ch, WORD Gain, WORD wFreqDiv)

- **Parameter:**

Ch : [Input] the A/D channel.
Gain : [Input] the Gain, refer to Section 3.1
wFreqDiv : [Input] the sampling rate is $2M/(wFreqDiv)$

- **Return:**

P100X_NoError : successful
P100X_INTStartError : failure

4.6.4 P100X_INT_AdStop

- **Description :**

This subroutine will stop the interrupt transfer and remove the installed interrupt handler.

- **Syntax :**

WORD P100X_INT_AdStop(void)

- **Parameter:**

None

- **Return:**

P100X_NoError : successful
P100X_INTStopError : failure

4.6.5 P100X_GetBuffer

- **Description :**

This subroutine will copy the transferred interrupted data into the user's buffer (in word format).

- **Syntax :**

WORD P100X_GetBuffer(DWORD dwNum, WORD wBuffer[])

- **Parameter:**

wNum : [Input] The total number to transfer to User's Buffer.

wBuffer : [Output] The address of wBuffer (Array of word) that will contain the hex A/D value.

The user must allocate sufficient space for this buffer. This function will fill the buffer with the data. The user can access the data after calling this function.

- **Return:**

P100X_NoError : successful

P100X_GetBufferError : failure

4.6.6 P100X_GetFloatBuffer

- **Description :**

This subroutine will copy the data into the user's buffer (in floating-point format).

- **Syntax :**

WORD P100X_GetFloatBuffer(DWORD dwNum, float fAdVal[])

- **Parameter:**

wNum : [Input] The total number of data points to transfer to the user's buffer.

fAdVal : [Output] Address of fAdVals (Array of float) that will contain the data as a voltage value(floating-point).

The user must allocate sufficient space for the buffer. This function will fill the buffer with the data. The user can access the data after calling this function.


- **Return:**


P100X_NoError : successful


P100X_GetBufferError : failure

4.6.7 Architecture of Interrupt mode

The flow chart below shows the steps for programming the A/D interrupt functions:

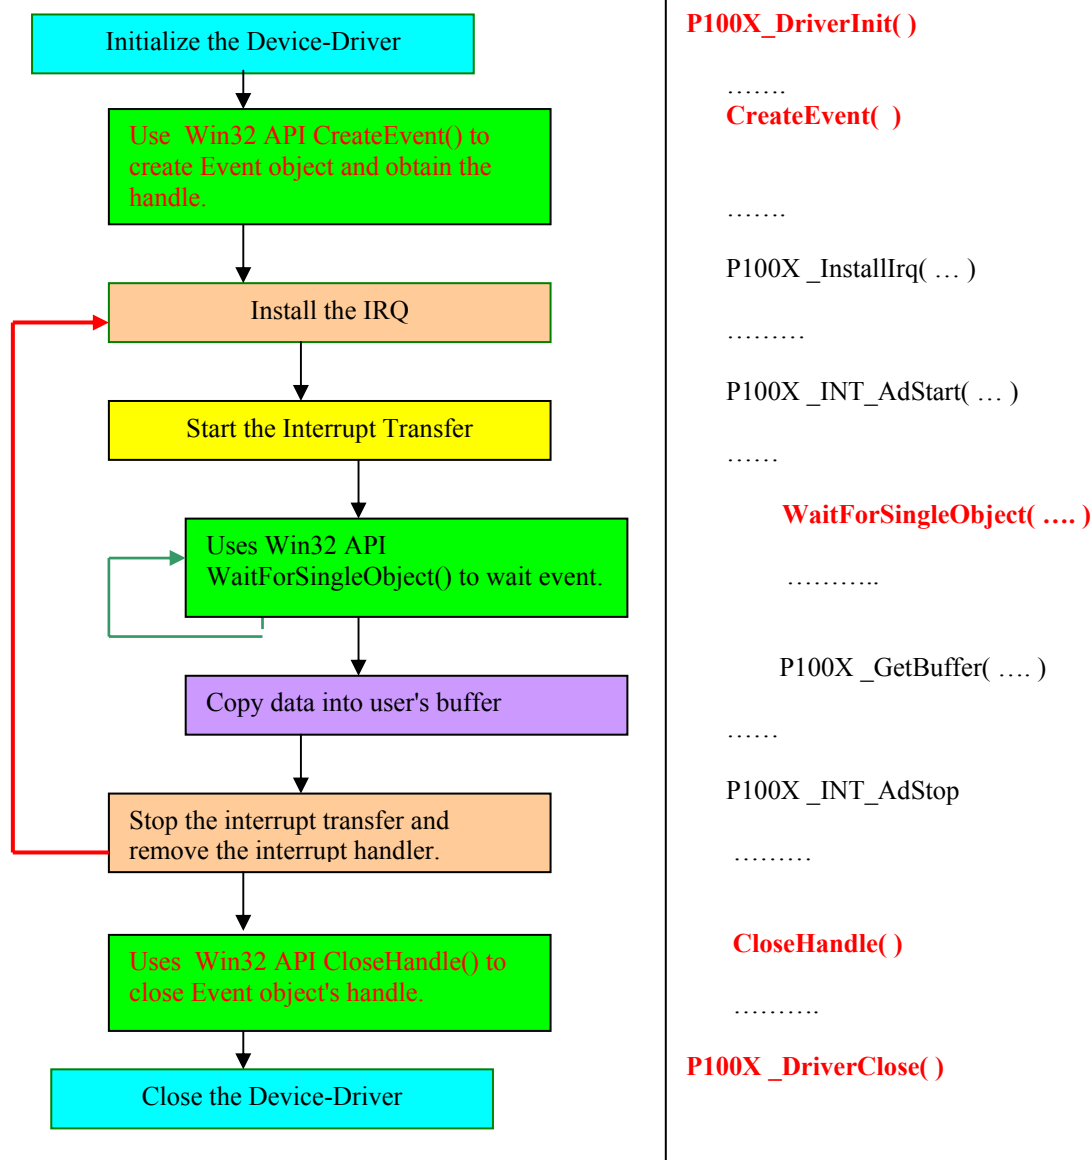

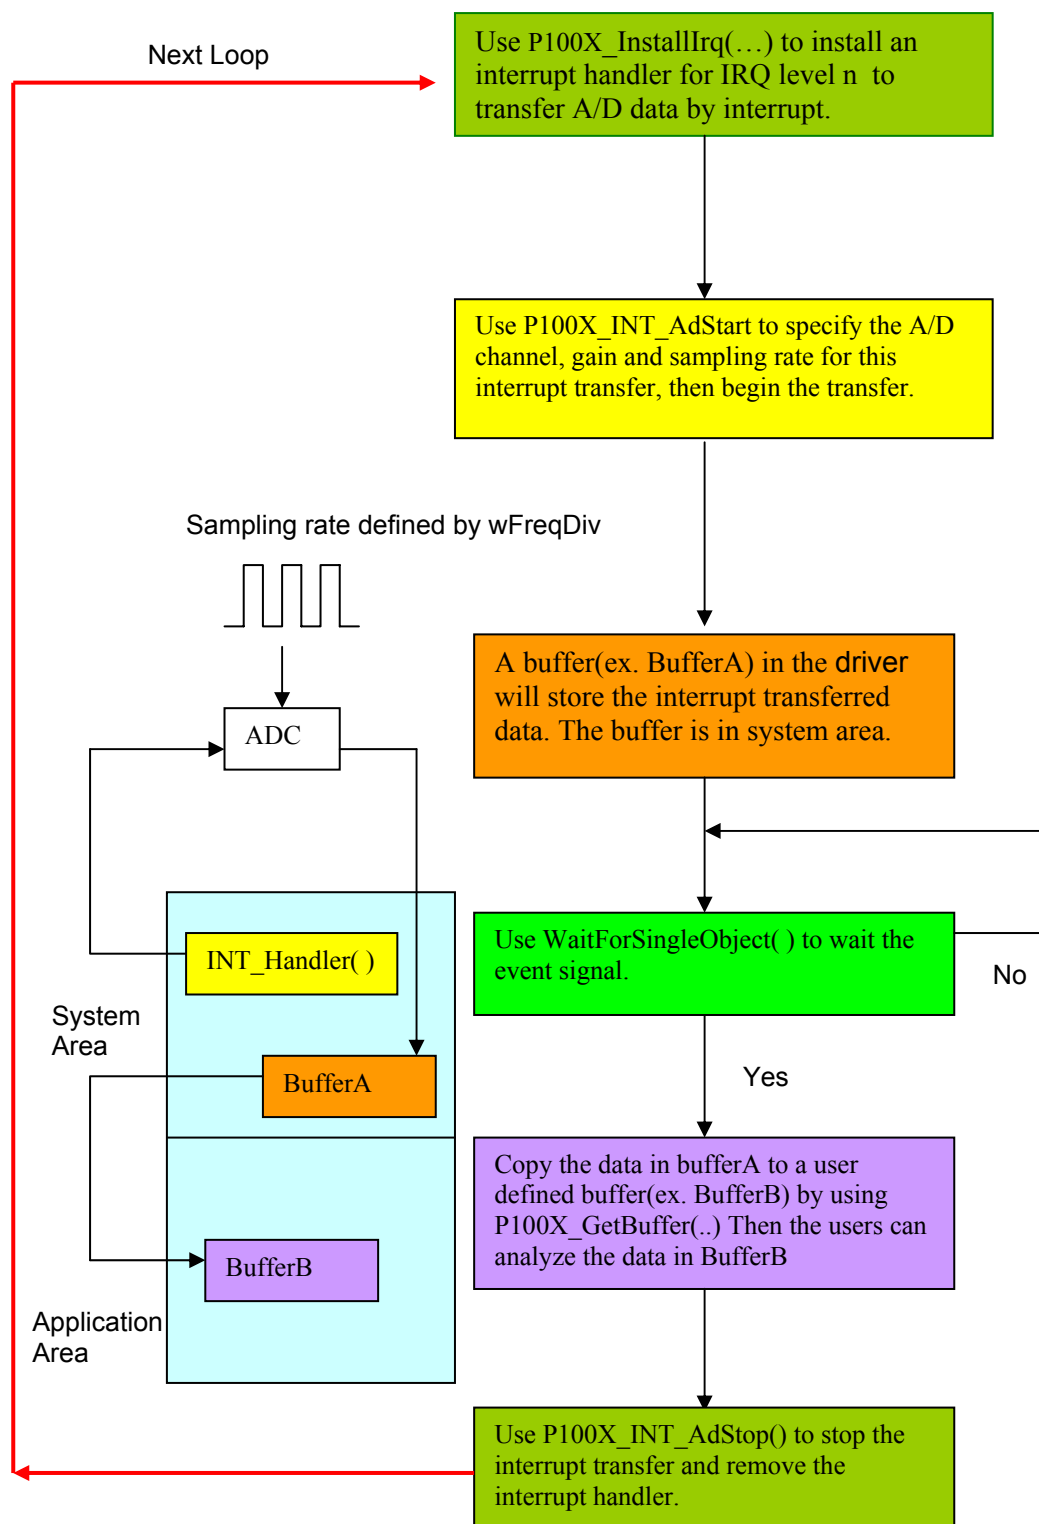

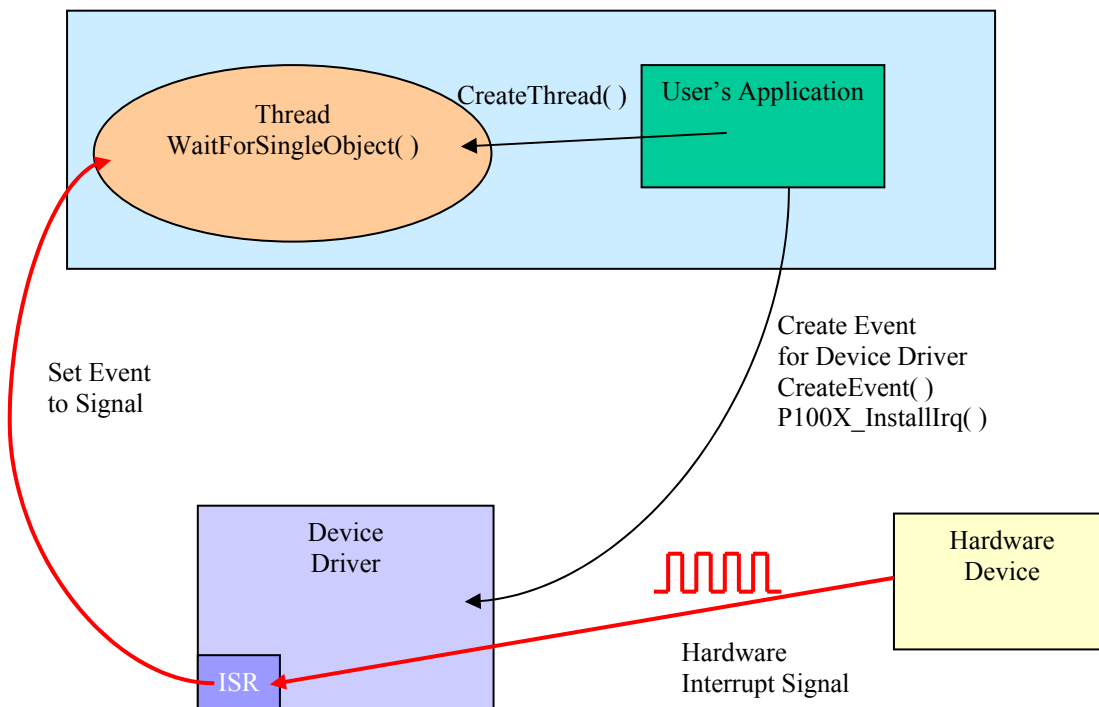

Please refer to the following Windows API functions:

The following descriptions of these functions were copied from MSDN. Refer to MSDN for complete details.

CreateEvent()

The CreateEvent function creates or opens a named or unnamed event object.

```

HANDLE CreateEvent(
    // pointer to security attributes
    LPSECURITY_ATTRIBUTES lpEventAttributes,
    BOOL bManualReset,      // flag for manual-reset event
    BOOL bInitialState,    // flag for initial state
    LPCTSTR lpName         // pointer to event-object name
);
  
```

CreateThread()

The CreateThread function creates a thread to execute within the virtual address space of the calling process.

To create a thread that runs in the virtual address space of another process, use the CreateRemoteThread function.

```
HANDLE CreateThread(  
    // pointer to security attributes  
    LPSECURITY_ATTRIBUTES lpThreadAttributes,  
    DWORD dwStackSize,      // initial thread stack size  
    // pointer to thread function  
    LPTHREAD_START_ROUTINE lpStartAddress,  
    LPVOID lpParameter,     // argument for new thread  
    DWORD dwCreationFlags,  // creation flags  
    LPDWORD lpThreadId      // pointer to receive thread ID  
);
```

WaitForSingleObject()



The WaitForSingleObject function returns when one of the following occurs:

- The specified object is in the signaled state.
- The time-out interval elapses.

To enter an alert-able wait state, use the WaitForSingleObjectEx function. To wait for multiple objects, use the WaitForMultipleObjects.

```
DWORD WaitForSingleObject(  
    HANDLE hHandle,          // handle to object to wait for  
    DWORD dwMilliseconds    // time-out interval in  
    milliseconds  
);
```

5. Program Architecture

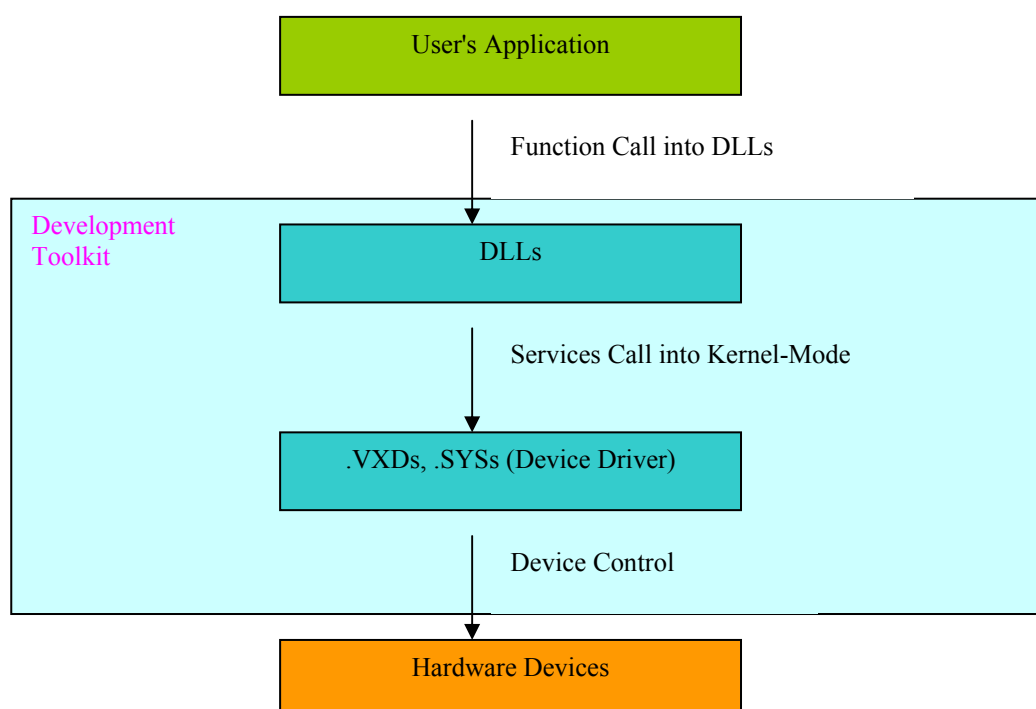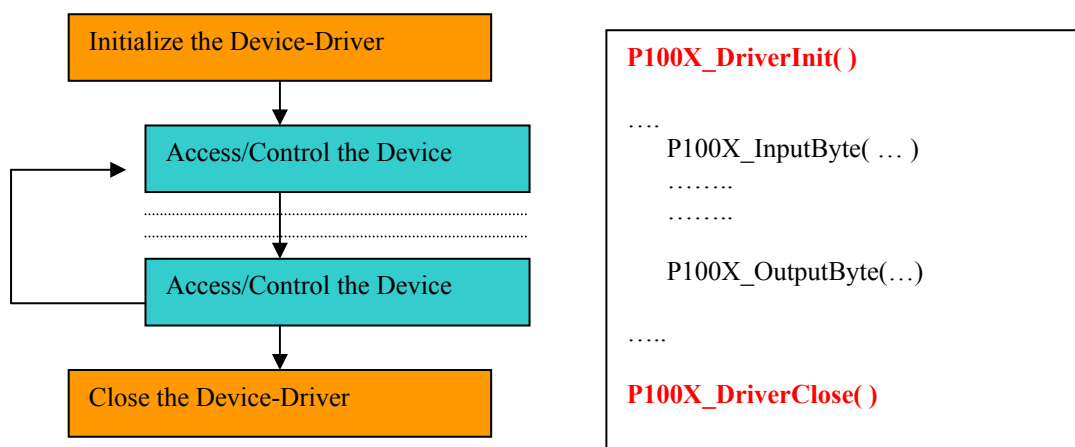

6. Reporting Problems

Technical support is provided at no charge you may contact us by telephone or email at

Telephone: 1-800-872-9436

Email: das@omega.com

When reporting problems, please include the following information:

- 1) Is the problem **reproducible**? If so, how?
- 2) What platform and version are you using? For example, Windows 3.1, Windows for Workgroups, Windows NT 4.0, etc.
- 3) Part number of the **product** that you are using?
- 4) If a dialog box with an **error message** was displayed, please include the full text of the dialog box, including the text in the title bar.
- 5) If the problem involves **other programs and/or hardware devices**, please provide a complete description of those items.
- 6) Other **comments** relative to this problem. Your **suggestions** are welcome.



WARRANTY/DISCLAIMER

OMEGA ENGINEERING, INC. warrants this unit to be free of defects in materials and workmanship for a period of 13 months from date of purchase. OMEGA's WARRANTY adds an additional one (1) month grace period to the normal one (1) year product warranty to cover handling and shipping time. This ensures that OMEGA's customers receive maximum coverage on each product.

If the unit malfunctions, it must be returned to the factory for evaluation. OMEGA's Customer Service Department will issue an Authorized Return (AR) number immediately upon phone or written request. Upon examination by OMEGA, if the unit is found to be defective, it will be repaired or replaced at no charge. OMEGA's WARRANTY does not apply to defects resulting from any action of the purchaser, including but not limited to mishandling, improper interfacing, operation outside of design limits, improper repair, or unauthorized modification. This WARRANTY is VOID if the unit shows evidence of having been tampered with or shows evidence of having been damaged as a result of excessive corrosion; or current, heat, moisture or vibration; improper specification; misapplication; misuse or other operating conditions outside of OMEGA's control. Components which wear are not warranted, including but not limited to contact points, fuses, and triacs.

OMEGA is pleased to offer suggestions on the use of its various products. However, OMEGA neither assumes responsibility for any omissions or errors nor assumes liability for any damages that result from the use of its products in accordance with information provided by OMEGA, either verbal or written. OMEGA warrants only that the parts manufactured by it will be as specified and free of defects. OMEGA MAKES NO OTHER WARRANTIES OR REPRESENTATIONS OF ANY KIND WHATSOEVER, EXPRESS OR IMPLIED, EXCEPT THAT OF TITLE, AND ALL IMPLIED WARRANTIES INCLUDING ANY WARRANTY OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE ARE HEREBY DISCLAIMED. LIMITATION OF LIABILITY: The remedies of purchaser set forth herein are exclusive, and the total liability of OMEGA with respect to this order, whether based on contract, warranty, negligence, indemnification, strict liability or otherwise, shall not exceed the purchase price of the component upon which liability is based. In no event shall OMEGA be liable for consequential, incidental or special damages.

CONDITIONS: Equipment sold by OMEGA is not intended to be used, nor shall it be used: (1) as a "Basic Component" under 10 CFR 21 (NRC), used in or with any nuclear installation or activity; or (2) in medical applications or used on humans. Should any Product(s) be used in or with any nuclear installation or activity, medical application, used on humans, or misused in any way, OMEGA assumes no responsibility as set forth in our basic WARRANTY/DISCLAIMER language, and, additionally, purchaser will indemnify OMEGA and hold OMEGA harmless from any liability or damage whatsoever arising out of the use of the Product(s) in such a manner.

RETURN REQUESTS/INQUIRIES

Direct all warranty and repair requests/inquiries to the OMEGA Customer Service Department. BEFORE RETURNING ANY PRODUCT(S) TO OMEGA, PURCHASER MUST OBTAIN AN AUTHORIZED RETURN (AR) NUMBER FROM OMEGA'S CUSTOMER SERVICE DEPARTMENT (IN ORDER TO AVOID PROCESSING DELAYS). The assigned AR number should then be marked on the outside of the return package and on any correspondence.

The purchaser is responsible for shipping charges, freight, insurance and proper packaging to prevent breakage in transit.

FOR WARRANTY RETURNS, please have the following information available BEFORE contacting OMEGA:

1. Purchase Order number under which the product was PURCHASED,
2. Model and serial number of the product under warranty, and
3. Repair instructions and/or specific problems relative to the product.

FOR NON-WARRANTY REPAIRS, consult OMEGA for current repair charges. Have the following information available BEFORE contacting OMEGA:

1. Purchase Order number to cover the COST of the repair,
2. Model and serial number of the product, and
3. Repair instructions and/or specific problems relative to the product.

OMEGA's policy is to make running changes, not model changes, whenever an improvement is possible. This affords our customers the latest in technology and engineering.

OMEGA is a registered trademark of OMEGA ENGINEERING, INC.

© Copyright 2002 OMEGA ENGINEERING, INC. All rights reserved. This document may not be copied, photocopied, reproduced, translated, or reduced to any electronic medium or machine-readable form, in whole or in part, without the prior written consent of OMEGA ENGINEERING, INC.

Where Do I Find Everything I Need for Process Measurement and Control? OMEGA...Of Course!

Shop online at www.omega.com

TEMPERATURE

- ☑ Thermocouple, RTD & Thermistor Probes, Connectors, Panels & Assemblies
- ☑ Wire: Thermocouple, RTD & Thermistor
- ☑ Calibrators & Ice Point References
- ☑ Recorders, Controllers & Process Monitors
- ☑ Infrared Pyrometers

PRESSURE, STRAIN AND FORCE

- ☑ Transducers & Strain Gages
- ☑ Load Cells & Pressure Gages
- ☑ Displacement Transducers
- ☑ Instrumentation & Accessories

FLOW /LEVEL

- ☑ Rotameters, Gas Mass Flowmeters & Flow Computers
- ☑ Air Velocity Indicators
- ☑ Turbine / Paddlewheel Systems
- ☑ Totalizers & Batch Controllers

pH/CONDUCTIVITY

- ☑ pH Electrodes, Testers & Accessories
- ☑ Benchtop / Laboratory Meters
- ☑ Controllers, Calibrators, Simulators & Pumps
- ☑ Industrial pH & Conductivity Equipment

DATA ACQUISITION

- ☑ Data Acquisition & Engineering Software
- ☑ Communications-Based Acquisition Systems
- ☑ Plug-in Cards for Apple, IBM & Compatibles
- ☑ Datalogging Systems
- ☑ Recorders, Printers & Plotters

HEATERS

- ☑ Heating Cable
- ☑ Cartridge & Strip Heaters
- ☑ Immersion & Band Heaters
- ☑ Flexible Heaters
- ☑ Laboratory Heaters

ENVIRONMENTAL MONITORING AND CONTROL

- ☑ Metering & Control Instrumentation
- ☑ Refractometers
- ☑ Pumps & Tubing
- ☑ Air, Soil & Water Monitors
- ☑ Industrial Water & Wastewater Treatment
- ☑ pH, Conductivity & Dissolved Oxygen Instruments